



Factory CRO

Verdiepende sessie klinisch onderzoek in de MDR

Perspectief van CRO

Klinische evaluatie en klinische studies

23 mei 2019

Niels van Tienen



Rijksoverheid

Ministerie van Volksgezondheid, Welzijn en Sport



Factory CRO

Major changes MDR

General

- From directive to regulation
- Requirements MEDDEV guidance documents in body text
 - MEDDEV 2.7/1 rev 4, Clinical Evaluation
 - MEDDEV 2.7/4, Guidance on Clinical Investigations
 - MEDDEV 2.7/3, Clinical Investigations - SAE reporting
 - MEDDEV 2.12, Post Market Clinical Follow-up
- Requirements harmonized standards in body text
 - Good Clinical Practice (ISO 14155:2011)


Concerning clinical investigations and clinical evaluation

- Reinforcement of the rules on clinical evidence
- Reassessment of all devices, even when on market (no grandfathering)
- Life cycle approach
- Active approach
- EUDAMED
- Coordinated assessment procedure for clinical investigations



Factory CRO

Guidance

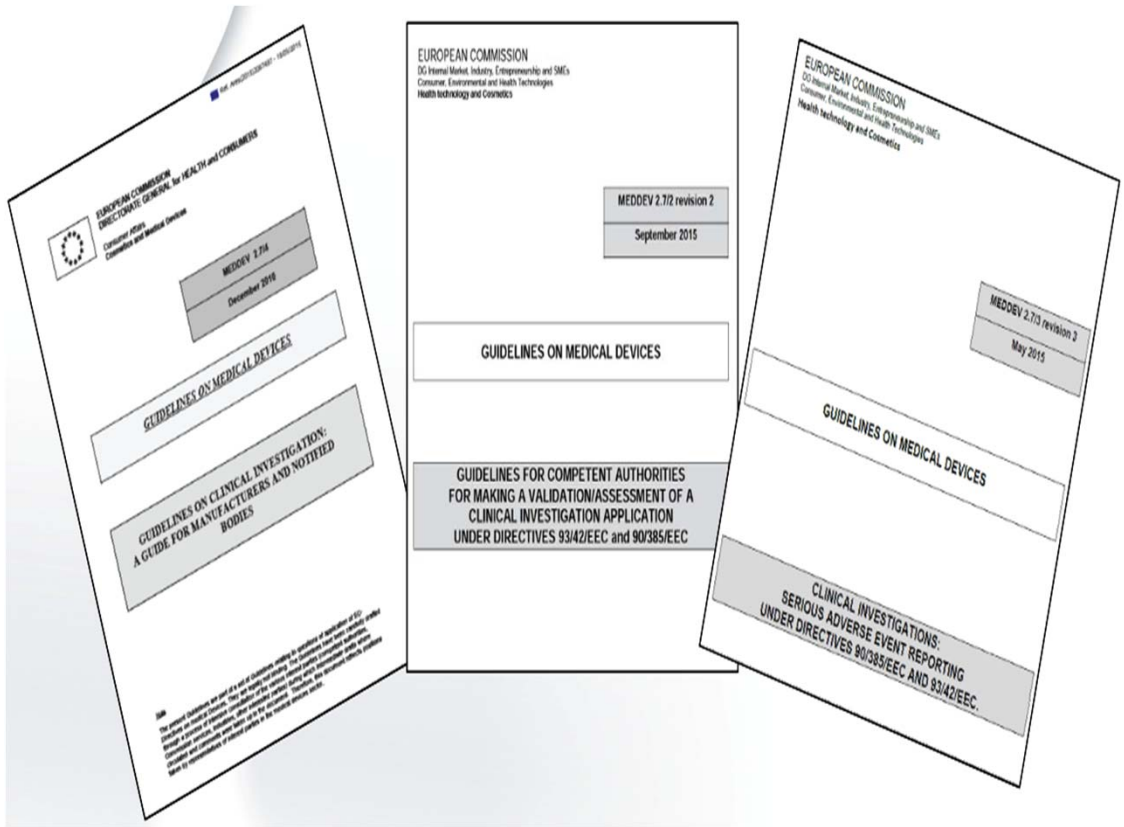

INTERNATIONAL STANDARD

ISO 14155

Second edition
2011-02-01

Clinical investigation of medical devices for human subjects — Good clinical practice

Investigation clinique des dispositifs médicaux pour sujets humains — Bonnes pratiques cliniques



Clinical investigations and Clinical Evaluation

MDR art 61: Demonstration of conformity with GSPR include a clinical evaluation

- Systematic and planned process to continuously generate, collect, analyse and assess clinical data pertaining to a device in order to verify the safety and performance, including clinical benefits, of the device when used as intended by the manufacturer

MDR art 62: Purpose of Clinical Investigations

- a) Verify device achieves performance intended by manufacturer
- b) Verify device establishes clinical benefits
- c) Verify device establishes clinical safety
 - Undesirable side effects
 - Acceptable risks benefit ratio

MDR art 64: Perform clinical investigations for implantables and class III

- a) Exempt when on market based on sufficient clinical data





Factory CRO

MDR Clinical Investigations

MDR art 62

- Conformity assessment
- No CE Mark
- EC / CA

MDR art 74

- Conformity assessment
- CE Mark
- Within / outside scope of intended purpose
- PMCF investigation
- EC / CA (notification in case not burdensome or extra invasive)

MDR art 82

- IIS (academic)
- EC (no negative vote)



ISO14155:2011 in 1 minute

- Standard - choice
- No certification – audited by third party

- Patient safety
- Data integrity

- Consent patients
- IP accountability / labelling
- Report SAEs
- Ensure training and qualification

- Comply with the CIP



MDR requirements Clinical Investigations

- Many MDR CI requirements similar to AIMDD, MDD, MEDDEV, ISO
 - CI in line with well-established international guidance (such as ISO14155:2011)
- Article 2(49): Introduction of sponsor
 - Investigators initiating IIS responsible for meeting MDR CI requirements
 - IIS valuable source of clinical evidence when sponsor is informed and trained on GCP requirements
- Article 62: Appoint legal representative
 - Sponsors not in EU
 - Responsible for ensuring sponsor obligations
- Annex XV: Appoint independent monitor (independent from site)
- Annex XV: Policy for FU of PD from CIP, prohibition of waivers
- Article 78: Coordinated assessment procedure
 - Single electronic application for multicentre CI in EUDAMED
 - Budget and timeline implications
 - MS to agree < 6 days which MS is coordinating
 - No agreement, proposed MS is coordinating
- Article 80: Report SAE with causal relationship to device, comparator or investigation procedure to MS without delay



Factory CRO

CRO observations

< # pivotal CI (CE marking)

- Sense holding pattern until NBs communicate decisions on clinical data collection / clinical strategy
- Other geographies

> PMCF CI

- Demand from NB including strict due dates
- Manufacturers reach out: I need to obtain clinical data for my NB / what kind of data? / clinical data

More sophisticated PMCF

- More site engagement
- Higher expectations regarding data points
- Better databases
- RBM

Manufacturers understand CEP > CER

- However still short term approach, even when CER interval 5Y

Manufacturers understand PMCF plan follows CER

- Still room for improvement
- Not just outline of future CI, data collection
- Alignment of documents, close gaps



Factory CRO

CRO observations

Feedback manufacturers: need of clinical expert to review CER

- Request from NB
- MEDDEV 2.7.1 rev 4, Annex VII, section 3.2.4 > NB requirement to have relevant clinical expertise including input from qualified medical practitioner

Conduct SoA literature review starting to become key concept

- Requirement for CEP, CER, CIP, IB under MDR and ISO14155:2019
- No longer background info for CI

For CRO EUDAMED is unclear

- Difficult to prepare manufacturer on database
- Difficult to prepare manufacturer on related procedures



Factory CRO

Clinical Evaluation Plan

Purpose

- Procedure future CE for device or family

Device description

- Classification
- Regulatory history
- Intended use
- Indication for use
- Intended users
- Intended clinical benefit
- Warnings precautions
- Clinical harms / risks
- Performance claims
- Safety claims

Equivalent devices

- Justification use of data



Clinical Evaluation Plan

SoA

- Alternative / conservative treatment
- Study end points alternative / conservative treatment
- Performancy and safety in studies alternative / conservative treatment
- Relevant outcome parameters
- Possible risks relevant for your device
- Pro's and con's of possible treatments (clinical benefit / unmet clinical need)

Identification of pertinent data

- Clinical Investigations
- PMCF plans
- PMS data

Analysis of data

- Compliance with GSPR
- Alignment with CER, IFU
- Risk management, residual risks, unanswered questions

Planning and responsibilities